


Bio TDB-100, TDB-120 Dry Block Thermostats

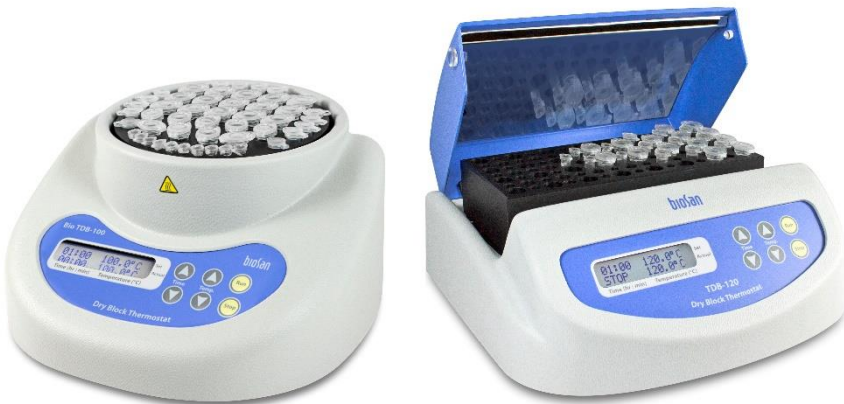

If you have any feedback on our products or services, we would like to hear from you.
Please send all feedback to:

Manufacturer:

SIA Biosan
Ratsupites 7 k-2, Riga, LV-1067, Latvia

Phone: +371 674 261 37

Fax: +371 674 281 01

<https://biosan.lv>

Marketing: marketing@biosan.lv

Service: service@biosan.lv

Contents

| | | |
|-----|--|----|
| 1. | About this edition of user instructions..... | 3 |
| 2. | Safety precautions | 4 |
| 3. | General information..... | 6 |
| 4. | Getting started..... | 7 |
| 5. | Operation | 8 |
| 6. | Calibration | 10 |
| 7. | Specifications | 11 |
| 8. | Ordering information | 12 |
| 9. | Care and maintenance | 13 |
| 10. | Storage and transportation..... | 13 |
| 11. | Warranty. Production date..... | 14 |
| 12. | EU Declaration of conformity..... | 15 |

1. About this edition of user instructions

1.1 The current edition of the user instructions applies to the following models:

| Model | Version |
|---|----------------------------|
| Bio TDB-100 , dry block thermostat | V.3AD, V.3AE |
| TDB-120 , dry block thermostat | V.7AD, V.7AE, V.8AD, V.8AE |

1.2 Edition 3.-8.02 – April of 2022

2. Safety precautions






Caution! Make sure you have fully read and understood the present Manual before using the equipment. Please pay special attention to sections marked by this symbol.



Caution! Surfaces can become hot during use. Always use thermal protective gloves to install or remove samples when the temperature is set higher than 60°C

2.1 Icons used on the unit and packaging

| | |
|---|---|
|  | CE marking, manufacturer affirms conformity with European health, safety, and environmental protection standards, see 12.1 |
|  | WEEE directive marking, see 12.1 |
|  | (TDB-120) Lid of the unit may become hot. Operate the lid by the safety handles on the sides. |

2.2 General safety

- The protection provided can be ineffective if the operation of the appliance does not comply with the manufacturer's requirements.
- The unit should be saved from shocks or falling.
- Store and transport the unit as described in section **10. Storage and transportation** on page 13.
- Before using any cleaning or decontamination methods except those recommended by the manufacturer, check with the manufacturer that the proposed method will not damage the equipment.
- Do not make modifications to the design of the unit.

2.3 Electrical safety

- Connect only to the mains with voltage corresponding to that on the serial number label.
- Do not plug the unit into an ungrounded power socket, and do not use an ungrounded extension lead.
- Ensure that the switch and the plug are easily accessible during use.
- If liquid penetrates into the unit, disconnect it from electric circuit and have it checked by a repair and maintenance technician.
- Disconnect the unit from electric circuit before moving.
- Do not operate the unit in premises where condensation can form. Operating conditions of the unit are defined in the section **7. Specification** on page 11.

2.4 During operation

- Use only tubes of standard size.
- Do not check the temperature by touch. Use a thermometer.
- Do not fill the tubes inside the unit.
- Do not operate the unit in environments with aggressive or explosive chemical mixtures. Please contact manufacturer for possibility of unit operation in specific atmosphere.
- Do not operate the unit if it is faulty or has been installed incorrectly.
- Do not use outside laboratory rooms.

2.5 Biological safety

- It is the user's responsibility to carry out appropriate decontamination if hazardous material is spilt on or penetrates into the equipment.

3. General information

Bio TDB-100 / TDB-120 – compact, easy-to-use thermostat for Eppendorf type microtubes. It is specially designed for long incubation at different temperatures. Thermostat has undeniable advantage working with microquantities of reagents in microtubes. The thermostat possesses unprecedentedly high precision and uniformity of temperature distribution over the block.

With the help of the software-enabled temperature calibration function, the user can calibrate the unit in the range of several percent of the selected temperature to compensate differences in the thermal behaviour of tubes from different manufacturers.

The thermostat can be used in:

| | |
|--|---|
| Molecular and gene engineering, cell biology | For PCR analyses, for temperature stabilisation in DNA/RNA restriction and denaturation reaction; |
| Biochemistry | For the enzyme processes analyses; |
| Microbiology | For the anaerobic microorganism cultivation, |
| Chemistry | For the preliminary heating of reagents in chromatography (especially when analysing chemical and biological components of fatty acids, which condense in cold micro syringes). |

Depending on the model, different quantities of microtubes of different volumes can be placed in the thermostat.

Table 1. Block capacity, by model

| Thermostat model | Microtube | | | |
|--------------------|-----------|--------|--------|--------|
| | 0.2 ml | 0.5 ml | 1.5 ml | 2.0 ml |
| Bio TDB-100 | 10 | 15 | 24 | |
| TDB-120 with A-53 | – | 21 | 32 | – |
| TDB-120 with A-103 | 100 | 21 | 32 | – |

For model Bio TDB-100, microtubes of 1.5 ml in volume fit in the sockets for 2.0 ml microtubes.

4. Getting started

4.1 **Unpacking.** Remove packing materials carefully and retain them for future shipment or storage of the unit. Examine the unit carefully for any damage incurred during transit. The warranty does not cover in-transit damage. Warranty covers only the units transported in the original package.

4.2 **Complete set.** Package contains:

- Dry block thermostat with aluminium block 1 pce.
- Spare fuse (inside fuse holder) 1 pce.
- Power cable 1 pce.
- User instructions 1 copy

4.3 **Setup.**

- Place the unit upon even horizontal non-flammable surface at least 20 cm away from any flammable materials;
- Remove protective film from the display;
- Plug the power cable into the socket on the rear side of the unit, and position it with easy access to the power switch and plug.

5. Operation

5.1 Recommendations during operation.



Please check the tubes before using, be sure that tubes are heat resistant. Do not heat the tubes over the melting point of the material they are made of. Remember that thin-walled tubes have a higher thermal conducting factor.

- Tube caps can open under the action of high temperature ($> 85^{\circ}\text{C}$), thus causing sample volume shrinkage or potential health risk when working with infected material. To prevent such cases, it is recommended to use tubes with cap lock of Safe-Lock[®] type.
- Do not fill tubes more than 3-5 mm over the level they are immersed in the heat block slot.

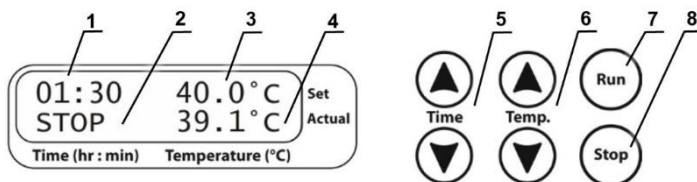


Figure 1. Control panel

5.2 Connect the power cord to a grounded power socket and switch ON (position I) the power switch located on the rear panel of the unit.

5.3 The unit will turn on and the following readouts will be shown on the display:

- Previously set time and temperature in the upper line (**Set**);
- Timer indication STOP and current temperature in the lower line (**Actual**).

5.4 **Temperature setting.** Use the ▼ and ▲ **Temp.** keys (fig. 1/6) to set the required temperature. Pressing the key for more than 2 s makes values change faster. Set temperature is displayed in the upper line of the display (fig. 1/3)

5.5 The heat block starts the heating. The actual temperature will be shown in the lower line of the display (fig. 1/4).

5.6 After thermal stabilisation of the unit (i.e., after the set and the current temperature equalize), place tubes into the block sockets.

5.7 **Time setting.** The unit is equipped with an independent timer for convenient control over the sample incubation time. Use the ▼ and ▲ **Time** keys (fig. 1/5) to set the required sample incubation time in hours and minutes (hh:mm). Pressing the key for more than 2 s makes values change faster. Set time is displayed in the upper line of the display (fig. 1/1)



Caution! (For model TDB-120) To avoid deformation of the lid, do not set the time longer than 8 h when setting the temperature above $+100^{\circ}\text{C}$.

5.8 Press the **Run** key (fig. 1/7) to start the timer. The elapsed time will be indicated in the lower line of the display (fig. 1/2). After the set time interval elapses, unit begins beeping and a blinking STOP indication shows on the display. Press the **Stop** key (fig. 1/8) to stop the signal.



Caution! Stopped timer does not stop the heating / temperature maintenance process. The heating can be stopped by lowering the temperature below 25°C using the ▼ **Temp** key (OFF indication shows on the display, fig.1/3).

- 5.9 The timer can be stopped before the set time interval elapses, if necessary, by pressing the **Stop** key. Press the **Run** key to restart the timer with the same time interval.
- 5.10 The set time interval can be changed at any time during the timer operation - just stop the timer and make the changes required.
- 5.11 If the working time is set to 00:00, the unit will operate non-stop.
- 5.12 After finishing the operation, switch OFF (position O) the unit with the power switch, unplug the power cord from electric circuit.

6. Calibration

- 6.1 The device is precalibrated at the factory (calibrating coefficient is 1.000) for operation with temperatures measured by a sensor in the heating block.
- 6.2 To change the calibration coefficient, hold the **Stop** key (fig. 1/8) pressed for more than 8 s to activate calibration mode. The calibration coefficient appears on the display (figure 4).







Figure 2. Display in calibration mode: 1. Calibration mode indicator; 2. Calibration coefficient; 3. Temperature with current coefficient


 **Note.** Values marked in grey on figures 2 and 3 are not used in calibration and are meant for service engineers.

- 6.3 **Restoring factory settings.** Set 1.000 value using the **▲** and **▼ Temp** keys (fig. 1/6) as shown on fig. 2/1 to restore the factory settings. Press the **Run** key (fig. 1/7) once to save the changes and exit the calibration mode.

 **Note.** Coefficient value changes are recommended after the unit has reached 30°C temperature.

- 6.4 **Calibration procedure.** To calibrate the unit, use an independent sensor with 0.5°C accuracy, which can fit in the cell in the block.
 - 6.4.1 Install the sensor into a cell in the block.
 - 6.4.2 Set the required temperature in operation mode (e.g., 40°C).
 - 6.4.3 After the unit reaches the set temperature (when the set and current temperature readings equal), leave the unit for 30 min for thermal stabilization.
 - 6.4.4 Let us assume that the reading of independent sensor is 39°C, but the display's actual temperature is 40°C. Then, it is necessary to add 1°C correction.
 - 6.4.5 Hold the **Stop** key pressed for more than 8 s to activate calibration mode (figure 2).
 - 6.4.6 Using the **▲** and **▼ Temp** keys, change the calibration coefficient (fig. 3/1) so that the new temperature value (fig. 3/2) corresponds to the independent sensor temperature. In our example, the calibration coefficient will be 0.974.

 **Note.** Calibration coefficient can be changed in range from 0.936 to 1.063 (±0.063, for model **Bio TDB-100**) or from 0.968 to 1.031 (±0.031, for model **TDB-120**), with increment of 0.001. This calibrating coefficient will correct temperature through all the operation range.

 **Note.** Coefficient value changes are recommended after the unit has reached 30°C temperature.

- 6.4.7 Press the **Stop** key once to save the changes and exit the calibration.
- 6.5 The display will show calibrated temperature as shown on fig. 4/1 and the unit will continue thermal stabilization according to the previously set temperature.




Figure 3. Changing the coefficient:
1. Calibration coefficient; 2. Temperature with current coefficient




Figure 4. Display after calibration:
1. Set temperature; 2. Current calibrated temperature

7. Specifications

The unit is designed for operation in cold rooms, incubators (excluding CO₂ incubators) and closed laboratory rooms at ambient temperature from +4°C to +40°C in a non-condensing atmosphere and maximum relative humidity 80% for temperatures up to 31°C decreasing linearly to 50% relative humidity at 40°C.

Biosan is committed to a continuous program of improvement and reserves the right to alter design and specifications of the equipment without additional notice.

| | Bio TDB-100 | TDB-120 |
|-----------------------------------|--|--------------------------------------|
| Temperature setting range | +25°C ... +100 °C | +25 °C ... +120 °C |
| Temperature regulation range | 5°C above RT ¹ ... +100°C | 5°C above RT ¹ ... +120°C |
| Temperature increment | 0,1°C | |
| Stability at +37°C | ±0,1°C | |
| Uniformity at +37°C | ±0,1°C | |
| Heat up time, from +25°C to +37°C | 4 min | |
| Internal thermal breaker | Yes | |
| Calibration option | Yes | |
| Calibration coefficient range | 0.936 – 1.063 (±0.063) | 0.968 – 1.031 (±0.031) |
| Heating block material | Aluminium | |
| Digital time setting | 1 minute - 96 hours or non-stop | |
| Display | 2x16 digit, LCD | |
| Dimensions | 210x230x115 mm | 230x210x110 mm |
| Working current | 120/220 V~, 50/60 Hz (see 8.1) | |
| Power and current consumption | 870 mA, 200 W | |
| Weight, accurate within 10% | 2.8 kg | |

¹ Room temperature

8. Ordering information

8.1 Models and versions available:

| Model | Block capacity | Version | Voltage, frequency | Catalogue number |
|-------------|---|---------|--------------------|------------------|
| Bio TDB-100 | Cylindrical/conical tubes, 10x0.2 ml, 15x0.5 ml, 24x1.5/2.0 ml | V.3AD | 220 V, 50/60 Hz | BS-010111-AAA |
| | | V.3AE | 120 V, 60 Hz | |
| TDB-120 | Block A-53 for conical tubes, 21x0.5 ml, 32x1.5 ml | V.7AD | 220 V, 50/60 Hz | BS-010135-AAA |
| | | V.7AE | 120 V, 60 Hz | |
| | Block A-103 for conical tubes, 50x0.2 ml, 21x0.5 ml, 32x1.5 ml | V.8AD | 220 V, 50/60 Hz | |
| | | V.8AE | 120 V, 60 Hz | |

9. Care and maintenance

9.1 Service.

9.1.1 If the unit is disabled (e.g., no platform motion, no reaction to key presses, etc) or requires maintenance, disconnect the unit from the mains and contact Biosan or your local Biosan representative.

9.1.2 All maintenance and repair operations (except listed below) must be performed only by qualified and specially trained personnel.

9.1.3 Operating integrity check. If the unit follows the procedure described in sections **5. Operation** and **6. Calibration**, then no additional checks are required.

9.2 Cleaning and disinfection.

9.2.1 Use mild soap and water with a soft cloth or sponge for cleaning the exterior. Rinse remaining washing solution with distilled water. Wipe dry the excess water with clean, soft cloth or sponge.

9.2.2 To disinfect the exterior plastic parts, use 75% ethanol or DNA/RNA removing solution (e.g., Biosan **PDS-250**). After disinfecting, wipe dry the surfaces.

9.2.3 The unit and its accessories are not autoclavable.

9.3 **Fuse replacement.** To replace the fuse, disconnect from electric circuit. Remove the power plug from the rear side of the unit. Pull out the fuse holder by applying leverage in recess (fig. 5/A). Remove the fuse from the holder. Check and replace with the correct fuse, if necessary, **M** 2 A for 220 V or **M** 3.15 A for 120 V, (type **M** - time lag: **Medium**).




Figure 5. Fuse replacement

9.4 **Disposal.** Disposal of the appliance requires special precautions and must be carried out at an appropriate disposal site, separate from normal household waste. To prevent pollution of the environment, all waste resulting from the disposal of the product must be collected and disposed of in the country of use, in accordance with the applicable requirements for the handling of electronic waste.

10. Storage and transportation

10.1 Store and transport the unit at ambient temperatures between -20°C and $+60^{\circ}\text{C}$ and maximum relative humidity of 80%.

10.2 After transportation or storage and before connecting it to the electric circuit, keep the unit under room temperature for 2-3 hrs.

10.3 For extended storage, the unit does not require special procedures.

11. Warranty. Production date

- 11.1 The manufacturer guarantees the compliance of unit with the requirements of specifications, if the customer follows the operation, storage and transportation instructions.
- 11.2 The warranted service life of unit from date of delivery to the customer is 24 months. For extended warranty, see **10.5**.
- 11.3 Warranty covers only the units transported in the original package.
- 11.4 If any manufacturing defects are discovered by the Customer, an unsatisfactory equipment report shall be compiled, certified and sent to the local distributor address. Please visit the **Technical support** section on our website at the link below to obtain the claim form.
- 11.5 Extended warranty. For **Bio TDB-100** and **TDB-120**, the *Basic Plus* class models, extended warranty is a paid service. Contact your local Biosan representative or our service department through the **Technical support** section on our website at the link below.
- 11.6 Description of the classes of our products is available in the **Product class description** section on our website at the link below.

Technical support



biosan.lv/en/support

Product class description



biosan.lv/classes-en

- 11.7 The following information will be required in the event that warranty or post-warranty service comes necessary. Complete the table below and retain for your records.

| Model | Serial number | Date of sale |
|--|---------------|--------------|
| Bio TDB-100 / TDB-120, dry block thermostats | | |

- 11.8 **Production date.** Production date is placed in the serial number, on the label of the unit. Serial number consists of 14 digits styled XXXXXYYMMZZZZ, where XXXXXX is model code, YY and MM – year and month of production, ZZZZ – unit number.

12. EU Declaration of conformity

12.1 Dry block thermostats **Bio TDB-100 & TDB-120** are in conformity with the following relevant Union legislations:

| | |
|--------------------------|---|
| LVD 2014/35/EU | LVS EN 61010-1:2011 Safety requirements for electrical equipment for measurement, control, and laboratory use. General requirements. LVS EN 61010-2-010:2015 Particular requirements for laboratory equipment for the heating of materials. |
| EMC 2014/30/EU | LVS EN 61326-1:2013 Electrical equipment for measurement, control and laboratory use. EMC requirements. General requirements. |
| RoHS3 2015/863/EU | Directive on the restriction of the use of certain hazardous substances in electrical and electronic equipment. |
| WEEE 2012/19/EU | Directive on waste electrical and electronic equipment. |

12.2 Declaration of Conformity is available for download on the page for the relevant model on our website by links below, in the **Downloads** section:



[Bio TDB-100](#)



[TDB-120](#)

SIA Biosan

Ratsupites 7 k-2, Riga, LV-1067, Latvia

Phone: +371 67426137 Fax: +371 67428101

<https://biosan.lv>

Edition 3.-8.02 – April of 2022